


### 

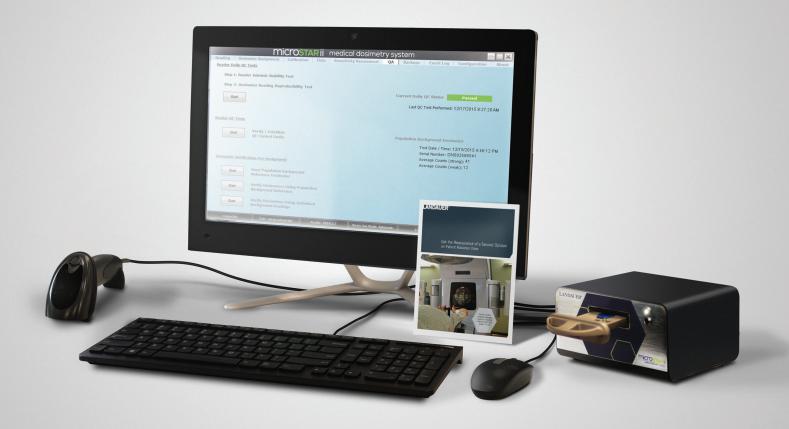

Use a simple, flexible medical dosimetry system to improve patient safety and quality

### Why Measure Patient Dose?

Patient safety in radiation oncology is the focus of public attention and regulatory scrutiny. Greater complexity of treatments and evolving standards are further raising the bar for radiation safety and increasing risk to health care organizations.

There are many reasons to independently verify planned dose during or prior to the first fraction of radiation treatment as part of a patient quality assurance program, including compliance with professional practice guidelines, risk reduction, and improved safety and quality of care.

Patient-specific dose measurements offer you important information for early identification and correction of potential errors or deficiencies in the delivery of prescribed dose. LANDAUER's Optically Stimulated Luminescence (OSL) technology, featuring nanoDot medical dosimeters and the microSTARii medical dosimetry system offer a simple, flexible, wireless alternative to diodes or mosfets for in vivo¹ dosimetry and can also be used with a QA phantom to verify machine output.



LANDAUER's OSL-Based Dosimeters, the most trusted technology for measuring occupational radiation dose, is customized for medical dosimetry applications

### microSTARii Medical Dosimetry System

# The microSTARii Medical Dosimetry reader using nanoDots is simple and efficient

- Immediate, independent verification of planned dose using nanoDot dosimeters
- Improved readout precision and durability with state-of-the-art pulsed OSL technology
- Fast, efficient single dosimeter readout near point of use
- Compact, lightweight and portable

# The microSTARii Medical Dosimetry System includes the following key components

- The microSTARii reader
- The microSTARii graphical user interface software on an included PC running Microsoft Windows.
- A 2D barcode scanner
- NanoDot Calibration and QC dosimeters



# Software customized to medical dosimetry applications for streamlined analysis, reporting and reimbursement

- Built-in and automated QC functionality for efficient implementation of the LANDAUER microSTAR reader Quality Assurance Program
- Patient-centric workflow, with additional fields for patient and exposure information automated re-reading capability for improved accuracy and efficiency
- Built-in dose reports to streamline reimbursement


Built-in dose reports to streamline reimbursement

### nanoDot Dosimeters

### A simple, flexible solution for measuring patient radiation dose

Since 1998, OSL technology has been trusted to measure occupational radiation dose for millions of health care professionals across the globe. OSL dosimeters are used for occupational dose monitoring in more than 80% of U.S. hospitals and are the focus of more than 30 published peer-reviewed scientific publications.

LANDAUER's nanoDot dosimeters, developed using proven OSL technology and the microSTARii medical dosimetry system is an effective tool for independent secondary verification of the quantity of dose delivered during radiation treatments. It allows you to mitigate risk for your facility.




- Wide operating energy range (5 keV to 20 MeV) makes nanoDot medical dosimeters an ideal solution for dose verification in radiation oncology and other point dose measurement applications
  - Linear dose response with dose up to 3 Gy, software-supported nonlinear calibration up to 15 Gy
- Reanalysis capabilities (nondestructive readout)
- Dosimeter preparation eliminated with single-use dosimeters
- Dosimeters are bar-coded for complete chain of custody
- Minimal angular or energy dependence in Megavoltage energy range



nanoDot Dosimeter

0 CM 1 2 3

- Accurate within ± 5.5% for photons and electrons from 5 MeV - 20 MeV\*
- Dosimeter can be placed anywhere on the body, is wireless, and radiolucent
- For measuring dose at a point of interest
- Can be used for in- and out-of-field measurements
- Can be used without buildup to make surface dose measurements or with buildup to make measurement at depth.\*\*



The nanoDot Medical Dosimeter is a compact, robust medical dosimeter ideal for a variety of dosimetry applications, such as secondary dose verification in radiation oncology and other point dose measurements

\* When reader is calibrated per recommended protocols and microSTAR QA program is implemented

\*\* The reader calibration must be consistent with the clinical use mode in terms of build-up characteristics

### Radiation Safety is a Team Effort

#### Your Clinical Team

- Provide quality patient care and outcomes
- Execute Quality Assurance program that reinforces patient safety initiatives
- Build trust in your community

### microSTARii Medical Dosimetry System

- Establish a continuous patient and instrumentation quality assurance program for radiological procedures
- Independently verify planned dose
- Simple, flexible, wireless solution for patient-specific dose measurements
- Tested and adopted by leading credentialing authorities for radiation dose measurement

### LANDAUER Implementation and QA Program Support

- In-house experts available for consultation to assist medical physicists implementing a new OSL-based medical dosimetry system
- For facilities without in-house medical physics expertise, LANDAUER's team of Qualified Medical Physicists can provide guidance on implementation of a medical dosimetry QA program that fits the unique requirements of your facility

### Radiation Oncology

Join leading radiation oncology authorities by choosing LANDAUER's state-of-the-art OSL technology for dose verification

#### **Radiological Physics Center**

For more than 30 years, the Radiological Physics Center in partnership with the National Cancer Institute has used a thermoluminescent dosimeter (TLD) for remote audits of photon and electron beam output, and energy verifications for electron beams, monitoring more than 1,700 radiation therapy facilities worldwide and measuring more than 13,000 beams annually. In 2010, after conducting a multi-year clinical evaluation of the technology, the RPC converted to use of OSL dosimeters in more than 90% of its remote audit program.

"If I could only buy one dose verification system, I would buy OSLD, because OSLD can do every measurement that TLD and diodes can do, plus measurements they cannot accurately capture."

ABOVE AND ASSOCIATION OF THE PROPERTY OF THE P

— Paul A. Jursinic

Paul A. Jursinic, Ph.D., noted physicist in quality assurance work, investigated a wide range of technologies. He compared measured dose with calculated dose output and concluded that OSLDs are a good substitute for TLDs and diodes for in vivo dosimetric measurements, particularly for surface dose measurements.<sup>3, 4</sup>

### **Dose Verification System Compared**

#### **TLD**

- Labor Intensive
- Time Consuming

#### **Diodes & Mosfets**

- Procedure-specific (multiple diodes needed for multiple energies)
- Wires may be obtrusive during use
- Not durable

#### **OSLD**

- Energy independent in therapy range
- Ideal for point dose measurements
- Proven superior accuracy and precision
- Simple, flexible and wirefree

#### nanoDot OSLD

Individually bar-coded nanoDot dosimeters enable complete chain of custody

### Learn More

Call 800-561-2708 or email inlightcustserv@landauer.com landauer.com

<sup>&</sup>lt;sup>3</sup> Jursinic, P.A., (2007) Characterization of optically stimulated luminescent dosimeters, OSLDs, for clinical dosimetric measurements. Medical Physics, 34(12):4594-604

<sup>&</sup>lt;sup>4</sup> Jursinic, P.A., (2015) Angular dependence of dose sensitivity of nanoDot optically stimulated luminescent dosimeters in different radiation geometries. Medical Physics, 42(10):5633-41